AvaMeter

INSTRUCTIONS FOR USE



Measure the distance from the incisive papilla to the **Resting Lip.**

The dental technician will position the incisal edge of the central incisors using this measurement.


Record your reading in millimeters



Measure the distance from the incisive papilla to the **Smiling Lip.**

This measurement helps determine the length of the central incisors.

Record your reading in millimeters

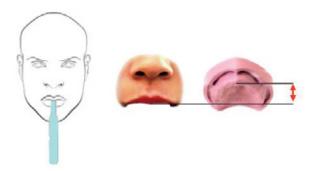

Submit all your records with your digital prescription through the AvaDent Dashboard and receive your Wagner Try-In.

Suggested Sterilization Procedure:

Clean AvaMeter using manual or automated (ultrasonic, washer/disinfector) methods. Place a cleaned AvaMeter in autoclave in a sterilization pouch that meets ISO 11140-1 standard for Class 1 Process indicators and meets ISO 111607 for pouch performance. *Gravity Method:* Heat for 30 minutes with a minimum temperature of 273° F completing the autoclave cycle recommended by autoclave manufacturer. *Pre-Vacuum Method:* Heat for 5 minutes at 273°F. Remove from sterilizer and confirm that sterilizing pouch indicates complete sterilization. Dry for 20 minutes.

